



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

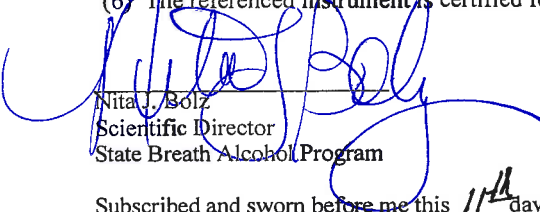
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

| | | | |
|--|---------------------|--|----------------------|
| Supervisor/Operator Performing the Verification Procedure: | | DataMaster cdm S/N | 130126 ✓ |
| Name | Michael Farmer | ID# | 6450 ✓ |
| | | Date | 12/24/10 ✓ |
| A | Agency | Anchorage Airport Police | Phone # 907-266-2411 |
| | Instrument Location | AAD DUI Processing Room | |
| B | Alco S/N | X301583 ✓ | Target Value .078 ✓ |
| | | High Pressure | 1300 |
| | Alco Test Values | .076 ✓ 1st Alco | .074 ✓ 2nd Alco |
| | Signature |  59  1/14/11 | |
| (OVER) | | | |


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 11th day of JAN, 2010.


 Daniel L. Nicholas
 Notary Public, State of Alaska
 Commission Expires with Office

(Notary Seal Stamp)



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130126

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130126

DECEMBER 24, 2010

OPERATOR'S NAME:

FARMER/MICHAEL/A

OPERATOR'S NUMBER: 6450

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI:

UOC

O.L. #: 1234567

DEPT/AGENCY: ANC6

CASE/REPORT: 10-1234

TEST TYPE: U

ALCO TARGET VALUE: .078

ALCO S/N: X301583

— BREATH ANALYSIS —

| | | |
|----------------------------|----------|-------|
| .078 ADJUSTED FOR 29.47 in | | |
| ALCO TARGET | .076 | 18:20 |
| BLANK TEST | .000 | 18:22 |
| INTERNAL STANDARD | VERIFIED | 18:22 |
| ALCO TV 29.47 in | .076 | 18:22 |
| BLANK TEST | .000 | 18:23 |
| SUBJECT SAMPLE | .000 | 18:23 |
| BLANK TEST | .000 | 18:24 |
| ALCO TV 29.47 in | .074 | 18:25 |
| BLANK TEST | .000 | 18:25 |

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130126

DECEMBER 24, 2010

TIME 18:25

— DIAGNOSTIC CHECK —

| | |
|------------------|----------|
| COMPUTER: | OKAY |
| PROGRAM: | OKAY |
| SOFTWARE DATE: | 02/20/01 |
| HEATERS | |
| SAMPLE CHAMBER: | 49c |
| BREATH TUBE: | 42c |
| BAROMETER: | 29.47 in |
| FLOW DETECTOR: | OKAY |
| PUMP | |
| HIGH SPEED: | OKAY |
| DETECTOR: | OKAY |
| FILTERS: | OKAY |
| QUARTZ STANDARD: | OKAY |
| CALIBRATION: | OKAY |

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrsuvwxyz{|}~■